

FIG. 1

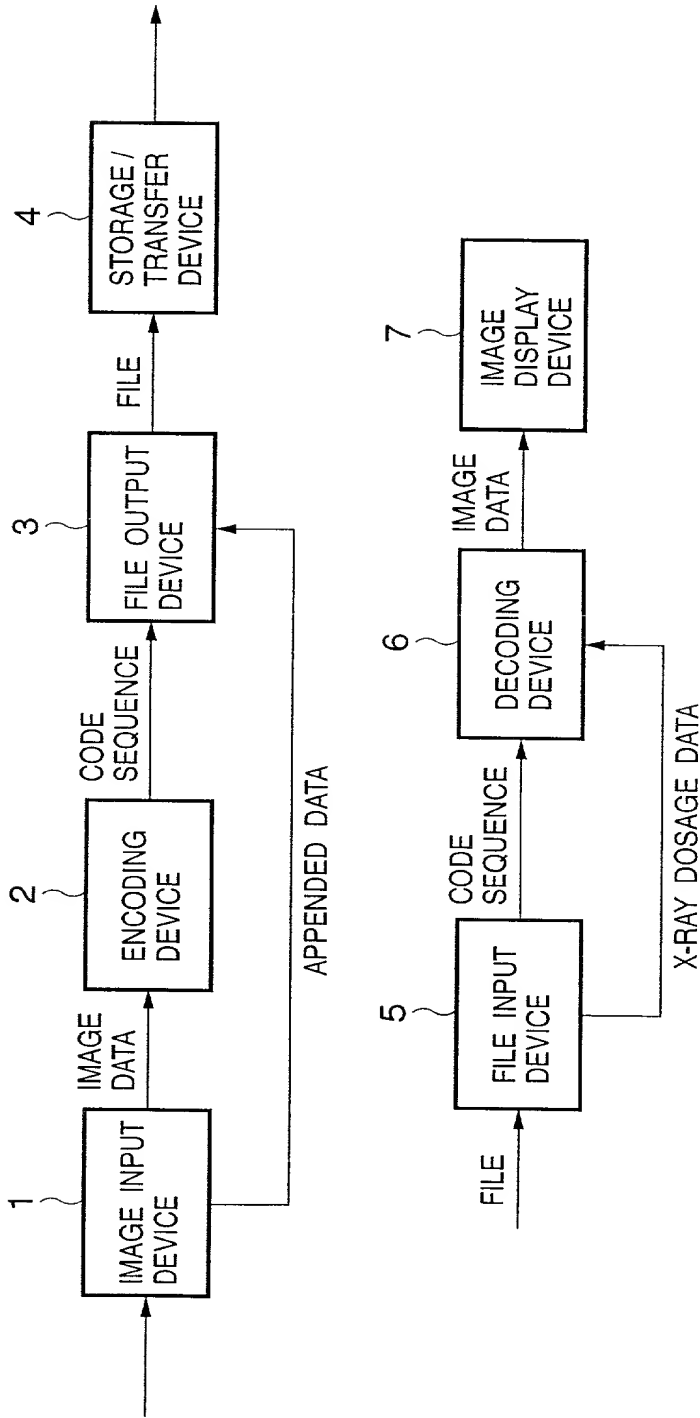


FIG. 2

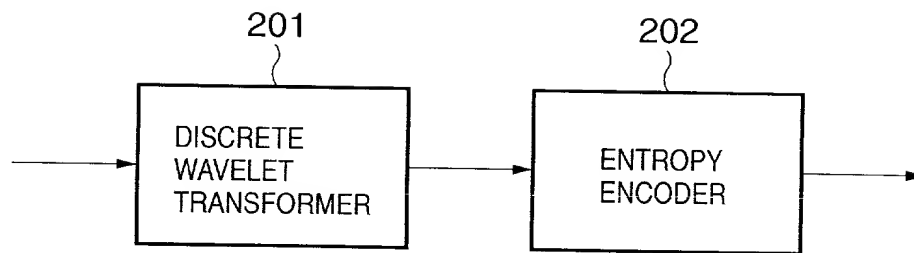


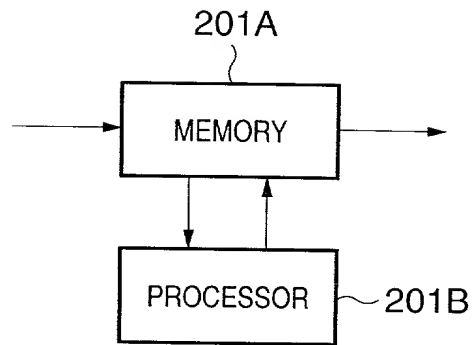
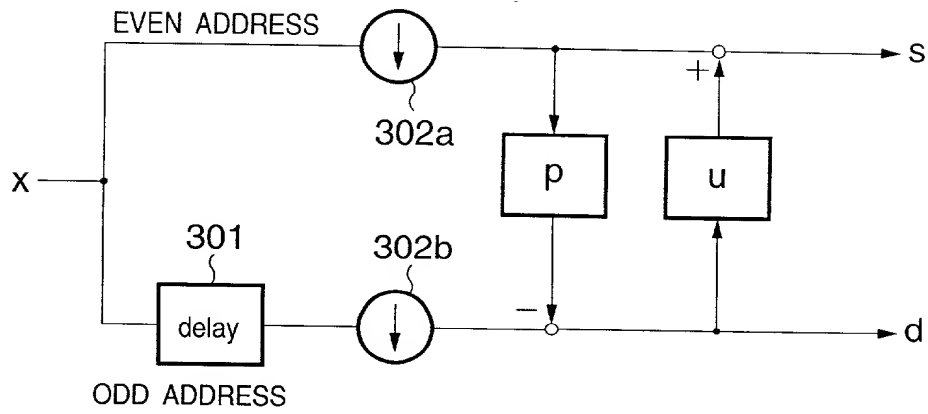
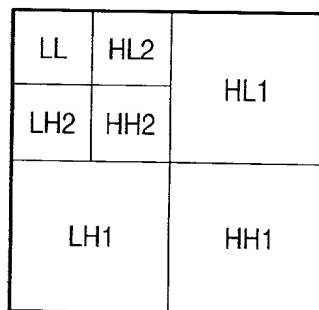
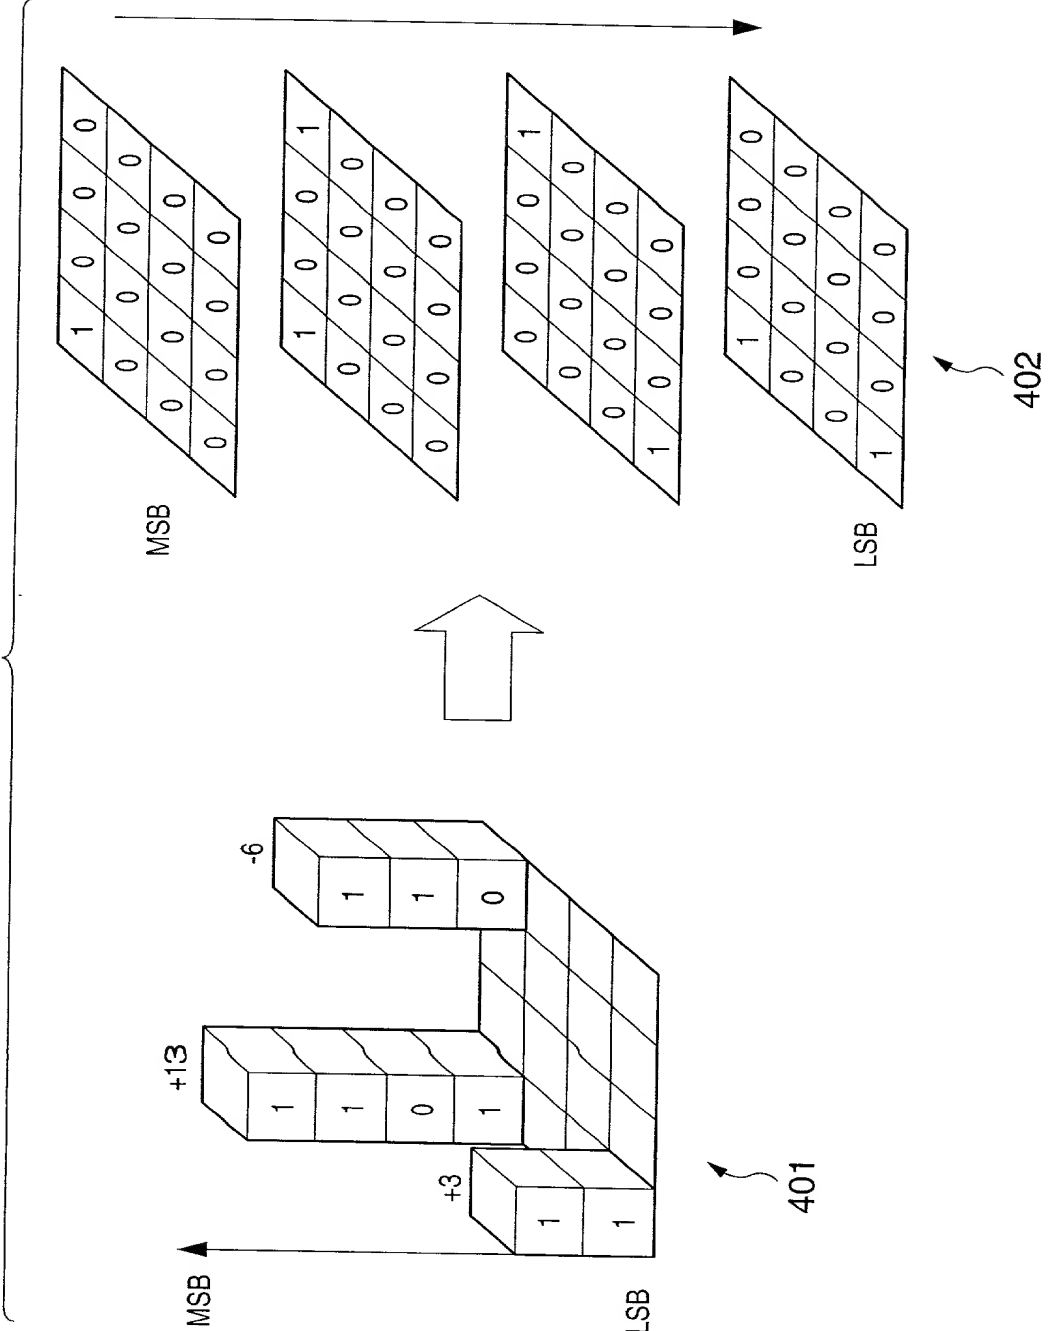
FIG. 3A**FIG. 3B****FIG. 3C**

FIG. 4






FIG. 5A




FIG. 5B




FIG. 5C

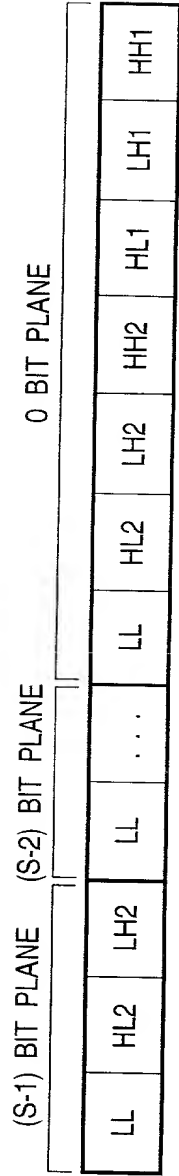


FIG. 5D

FIG. 6

PATIENT'S NAME	IMAGE SENSING DATA	X-RAY DOSAGE	CODE SEQUENCE
----------------	-----------------------	--------------	------------------

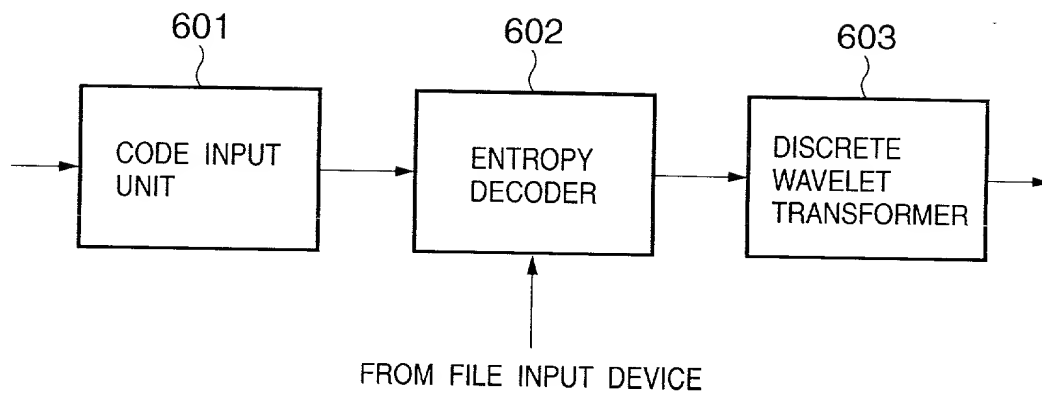
FIG. 7

FIG. 8

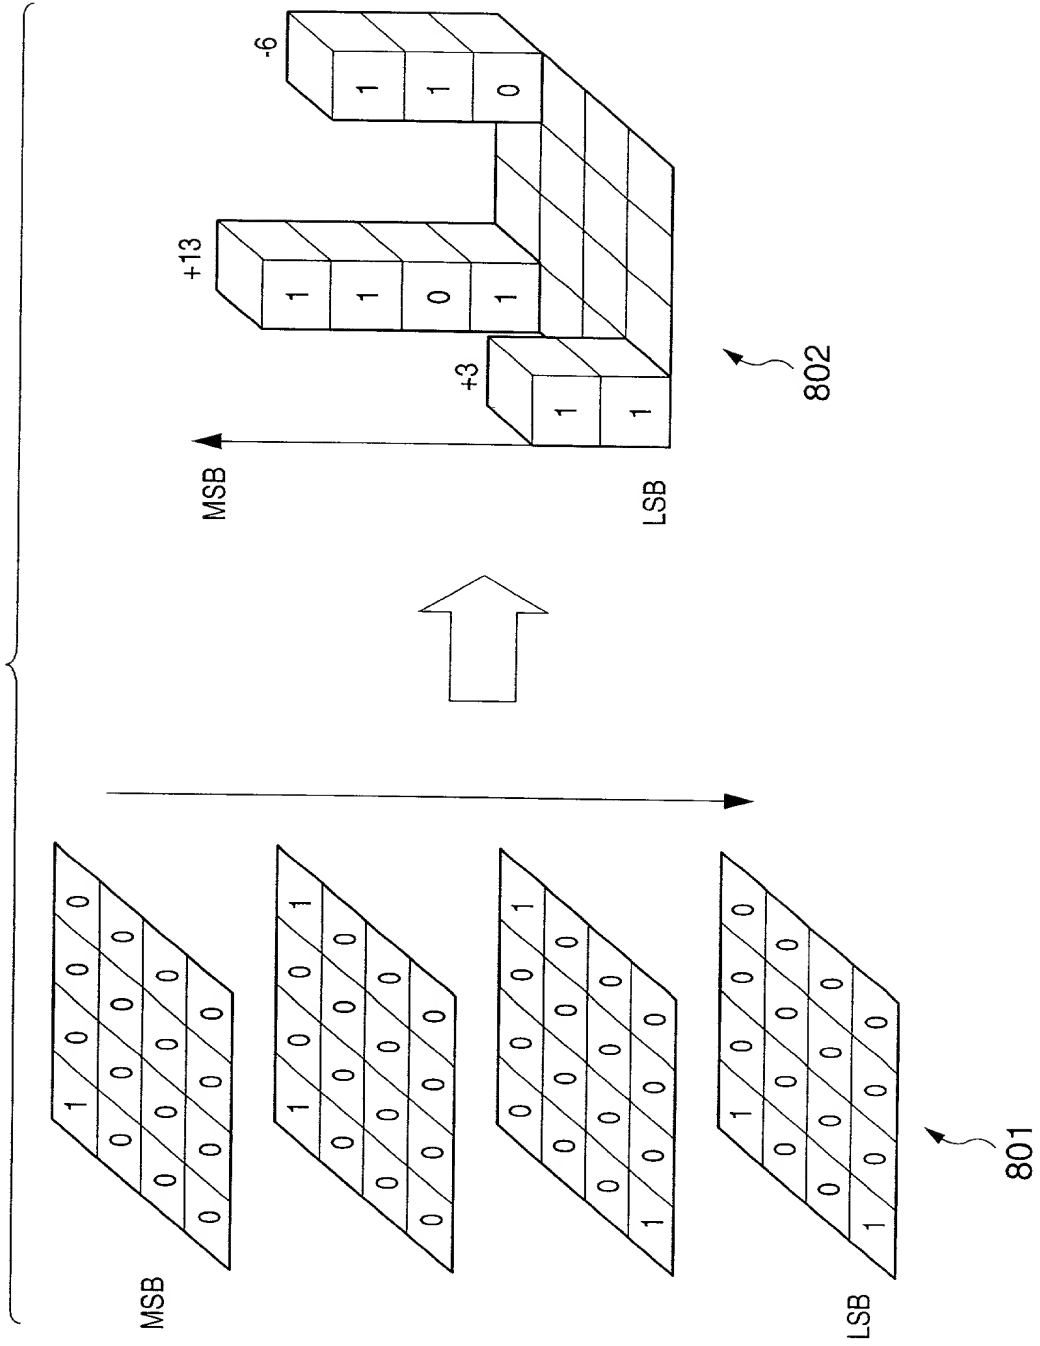


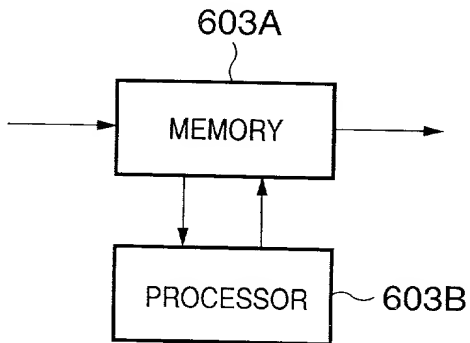
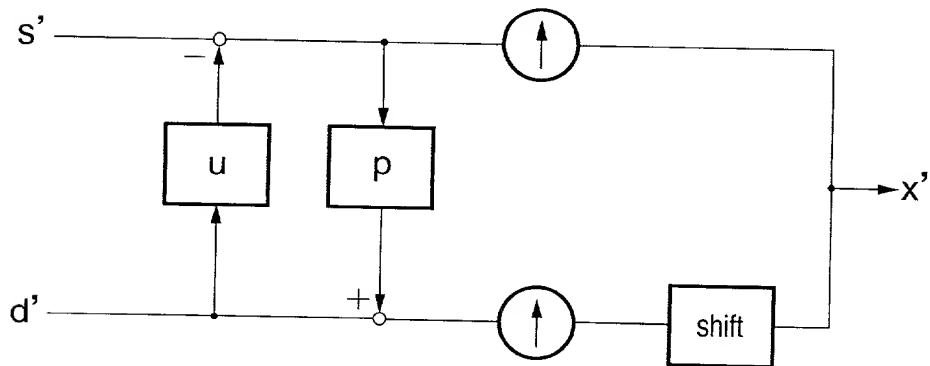
FIG. 9A**FIG. 9B**

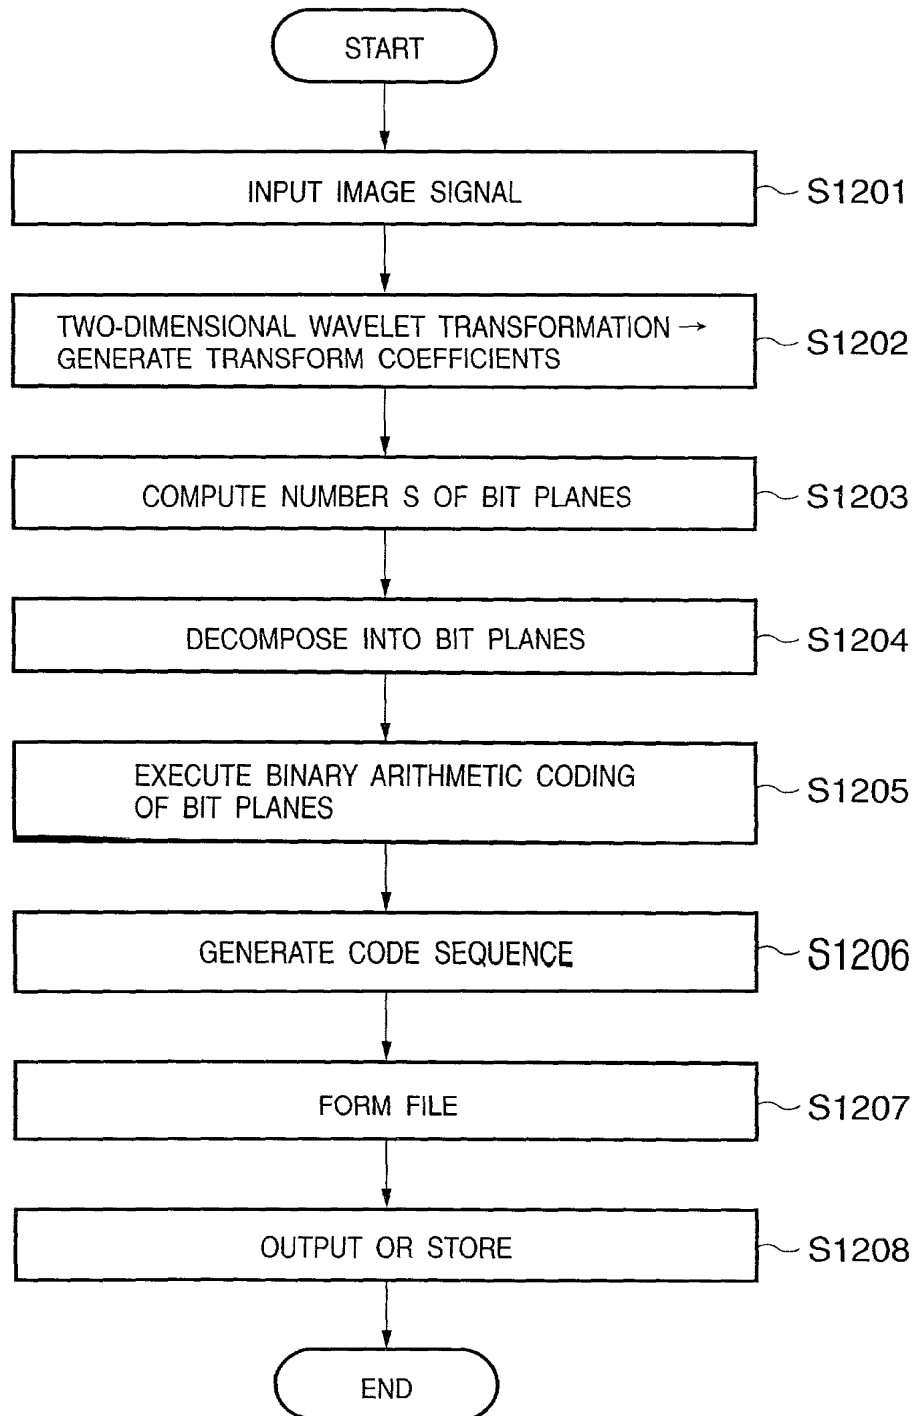
FIG. 10

FIG. 11

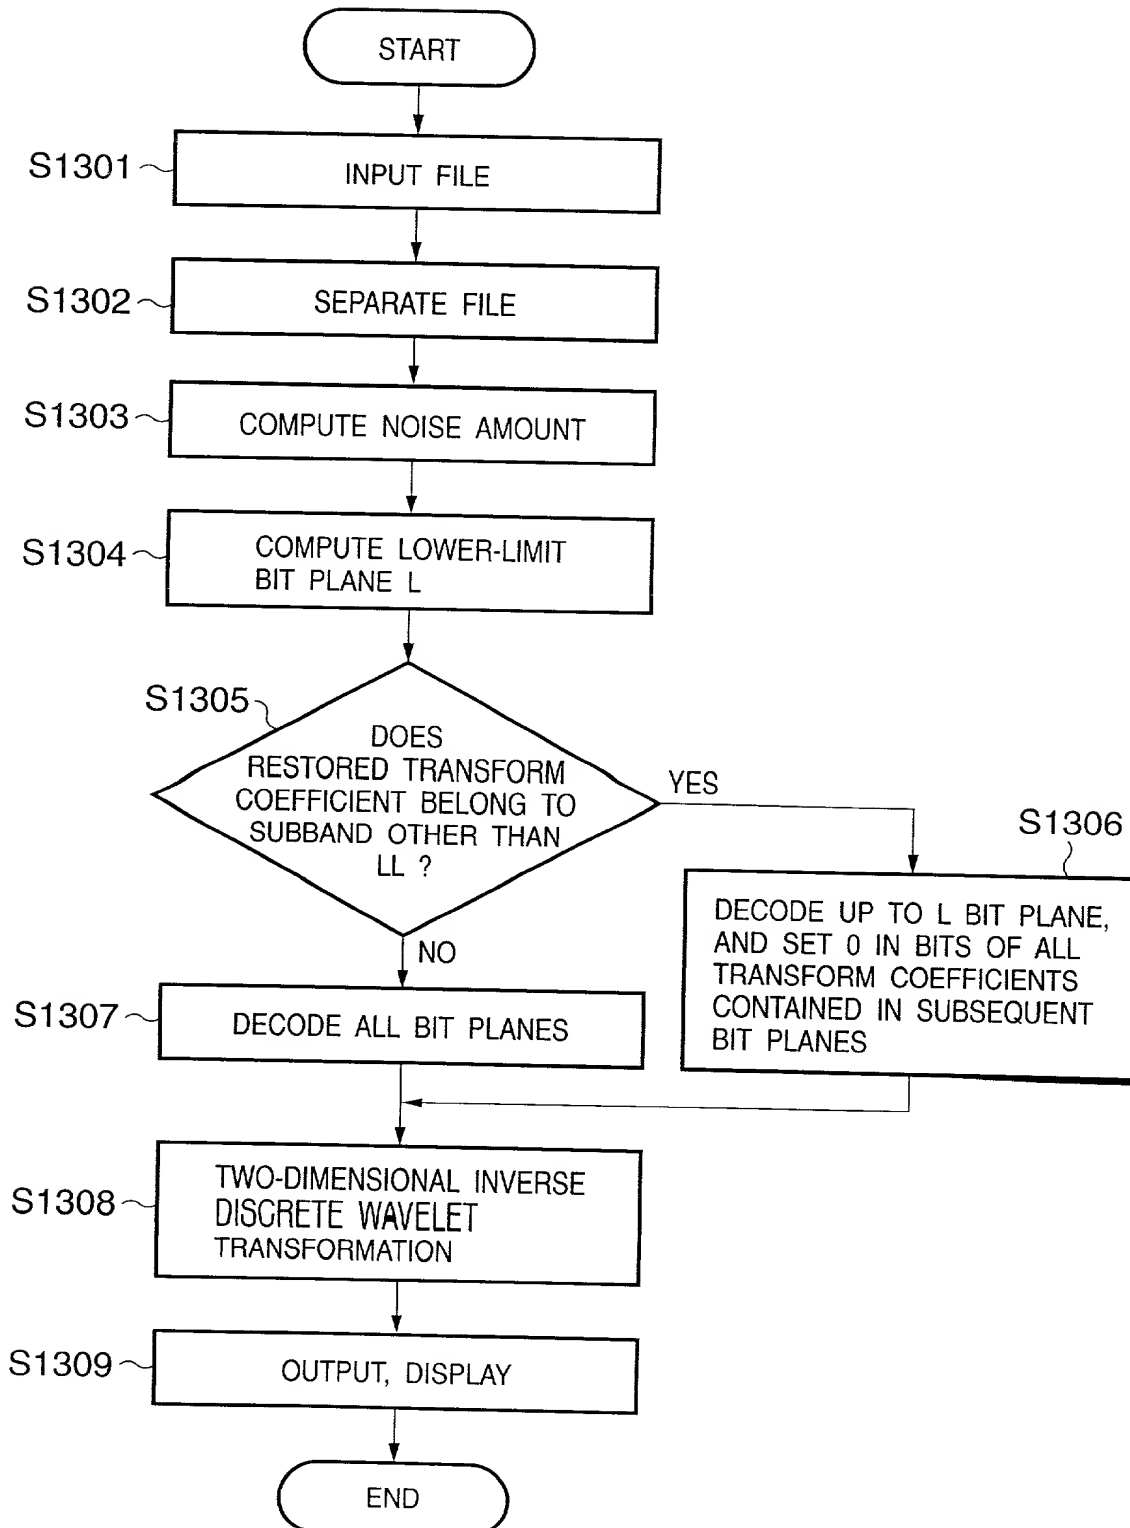


FIG. 12

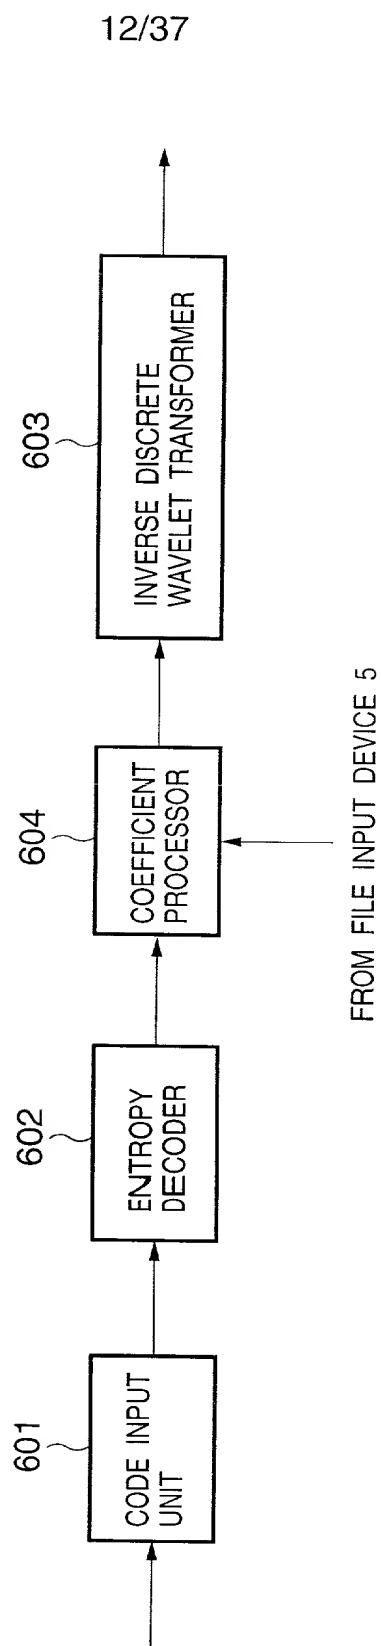


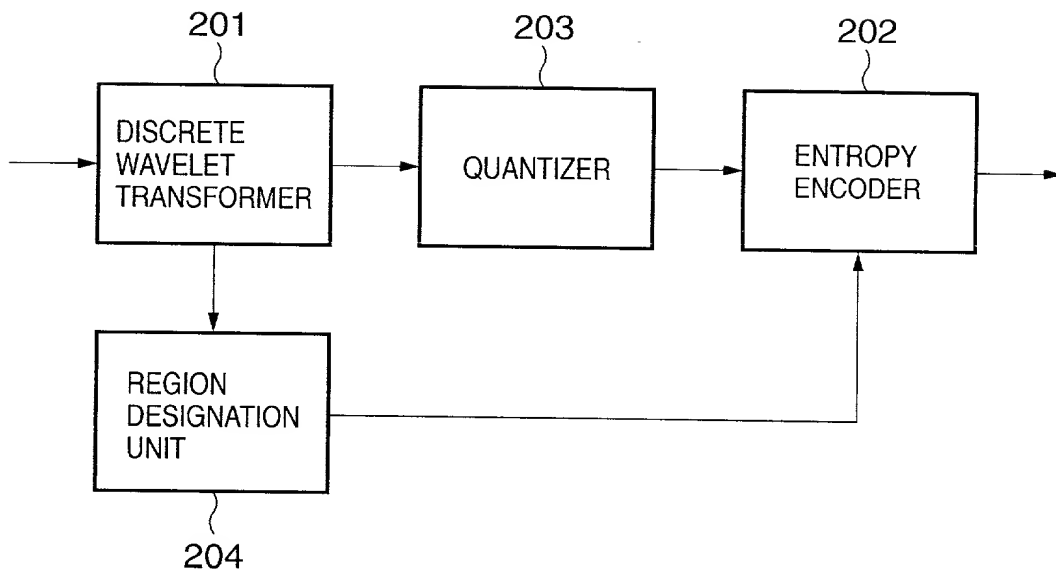
FIG. 13

FIG. 14A

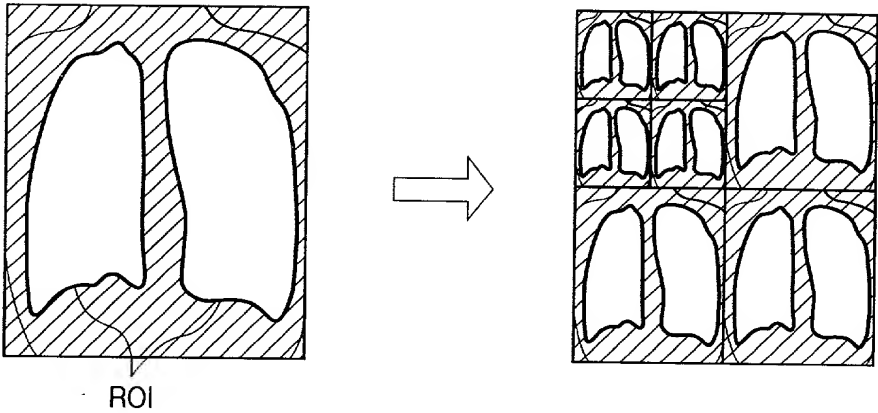


FIG. 14B

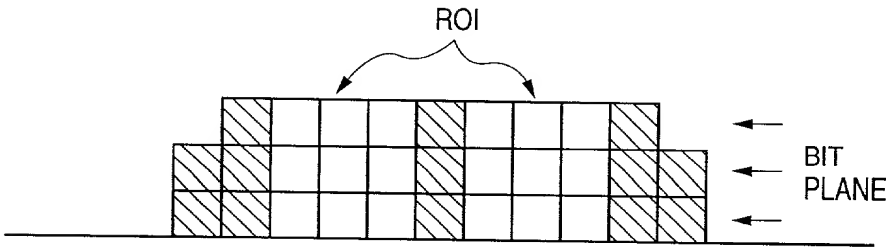


FIG. 14C

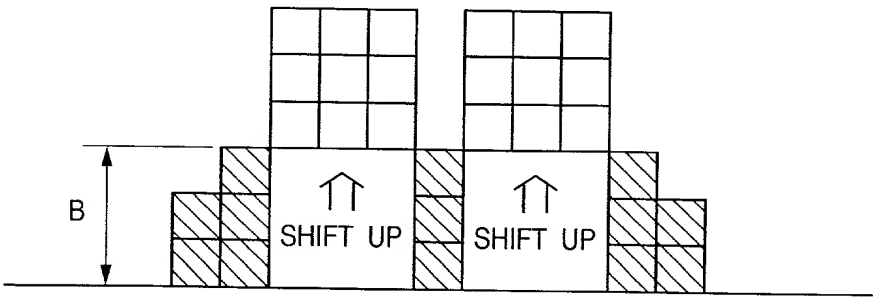


FIG. 15A

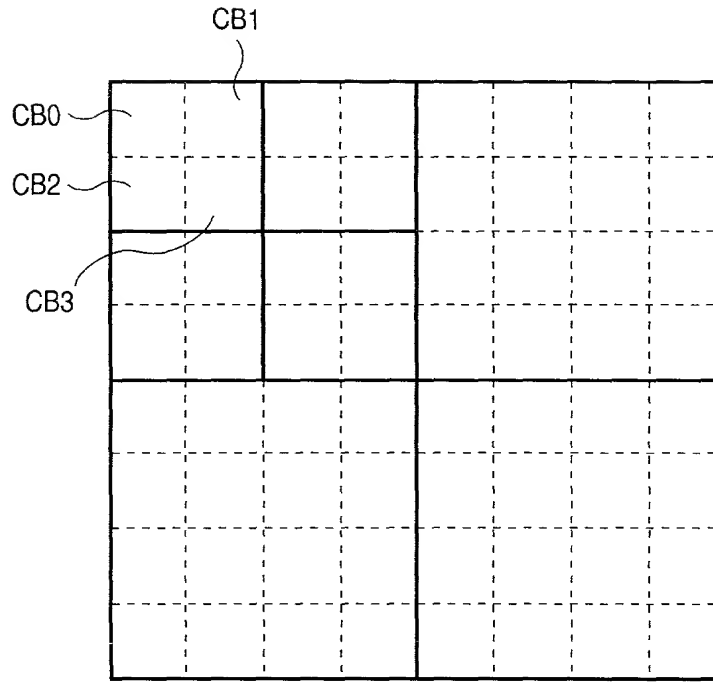
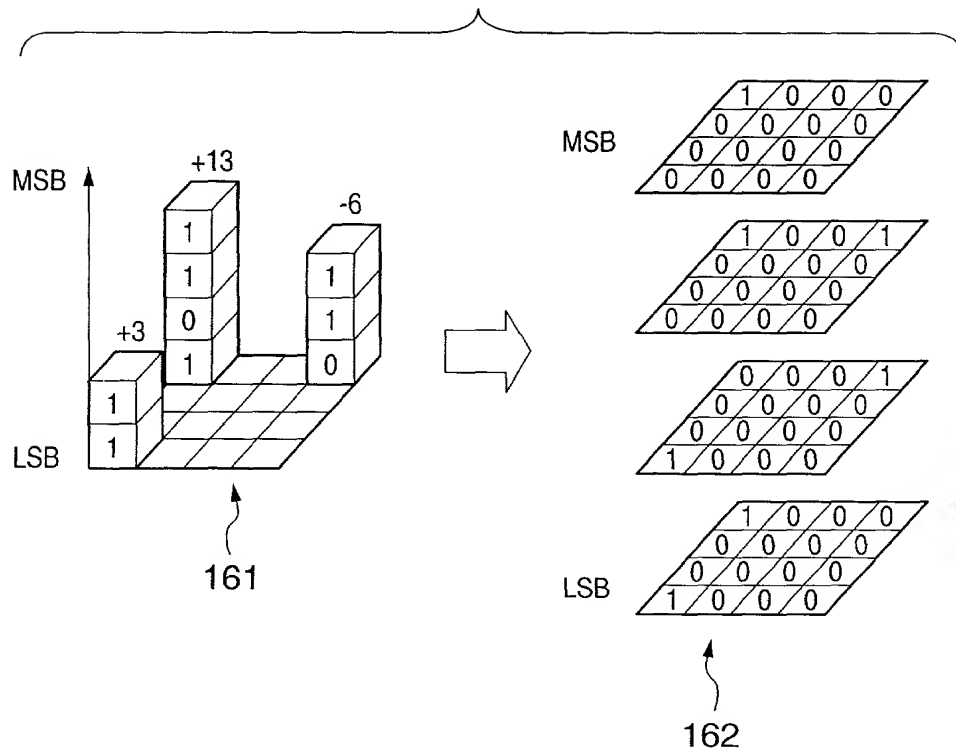


FIG. 15B






FIG. 16A




FIG. 16B



FIG. 16C

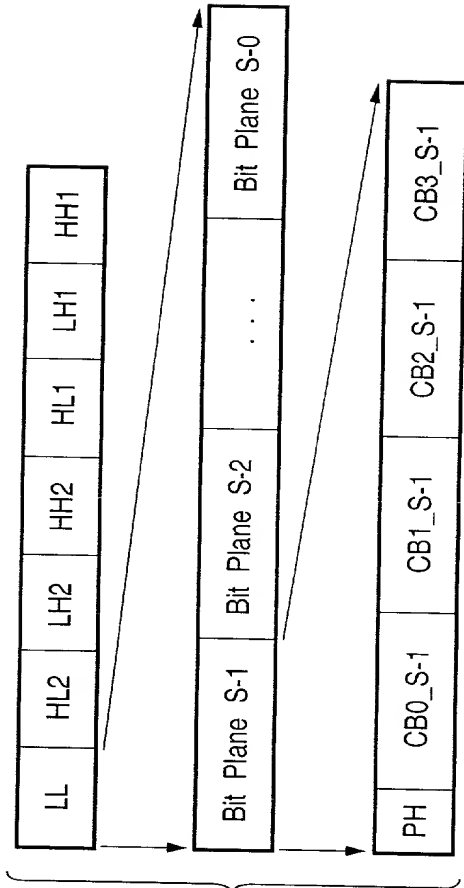


FIG. 16D

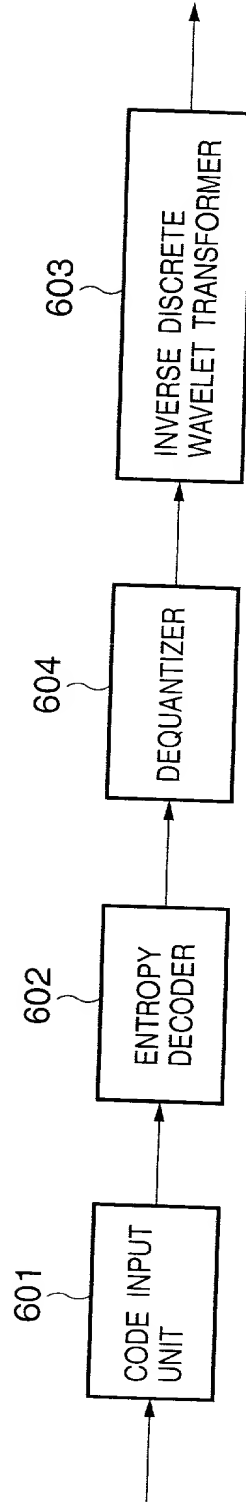


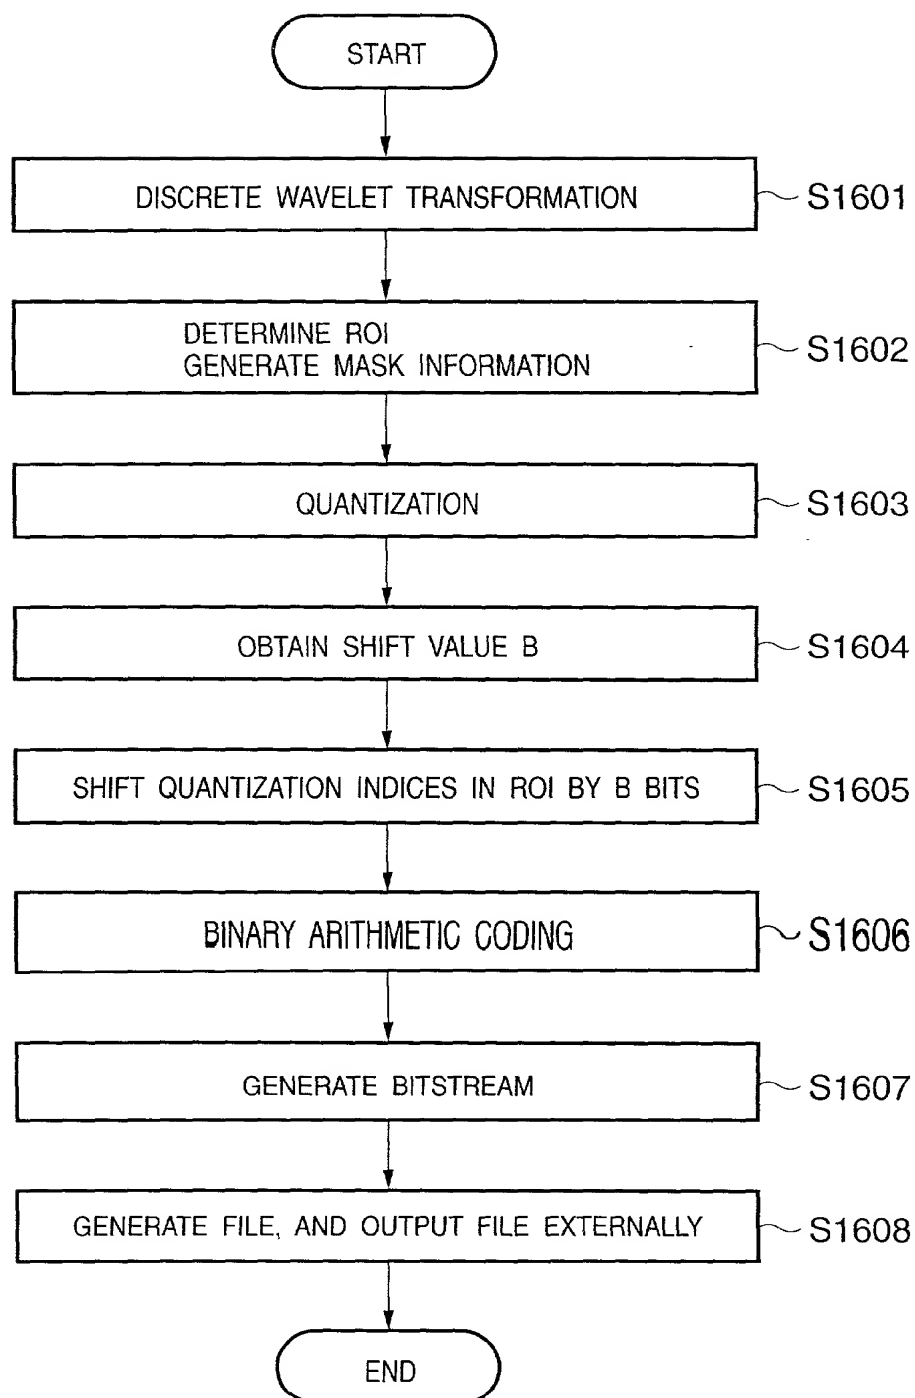
FIG. 18

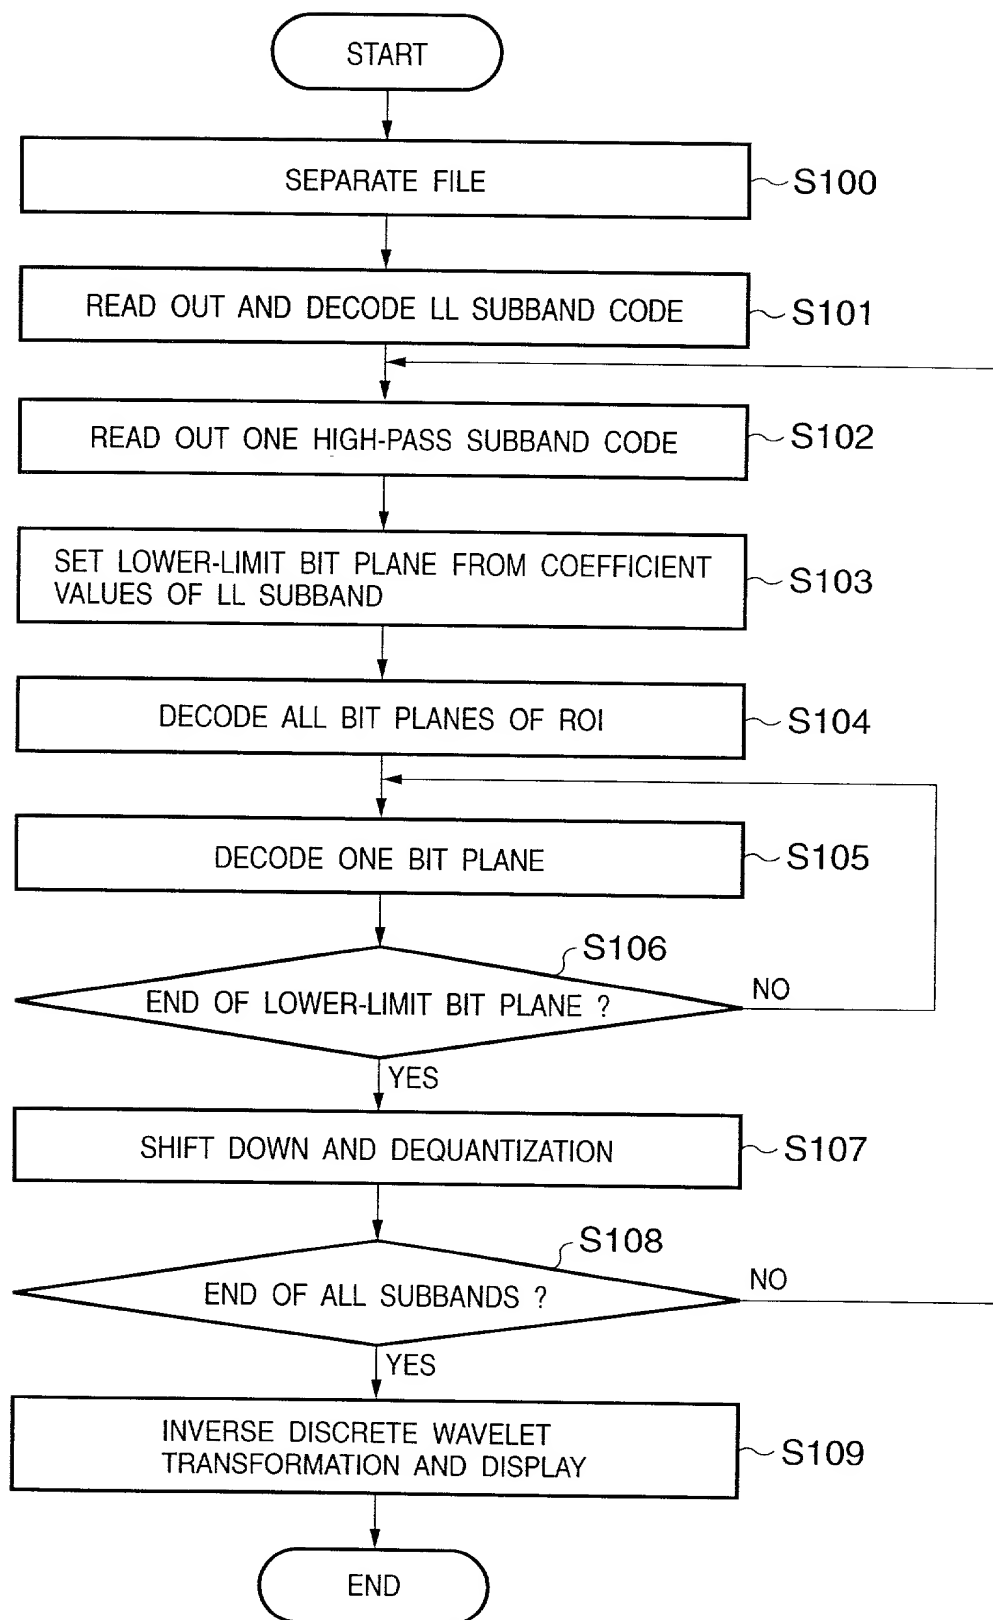
FIG. 19

FIG. 20A

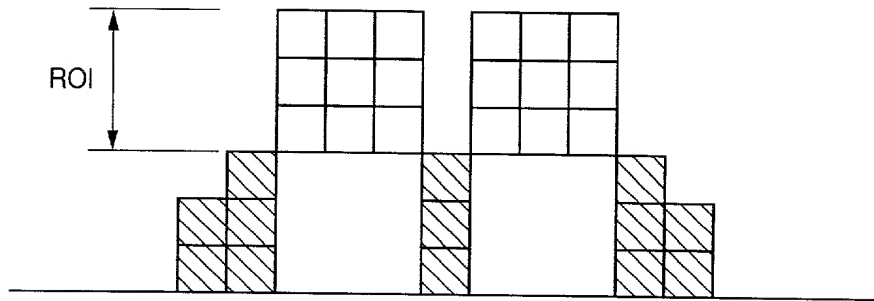


FIG. 20B

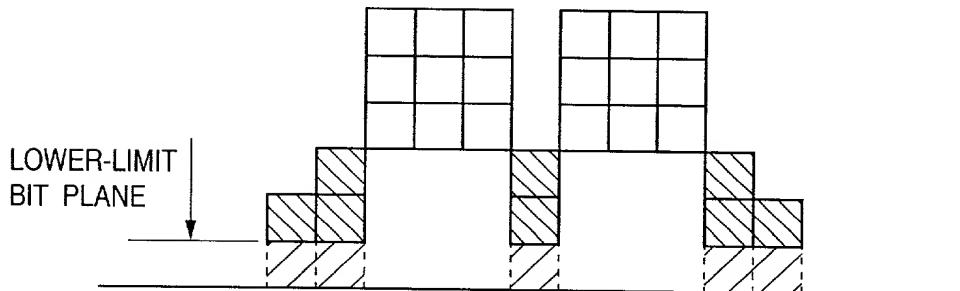


FIG. 20C

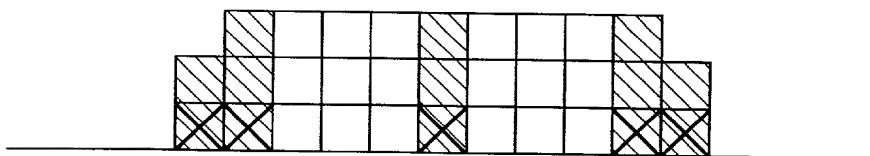


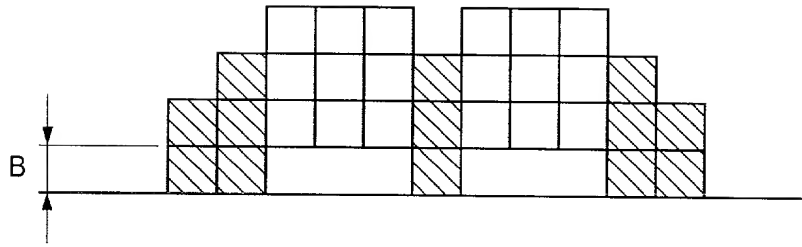
FIG. 21

FIG. 22

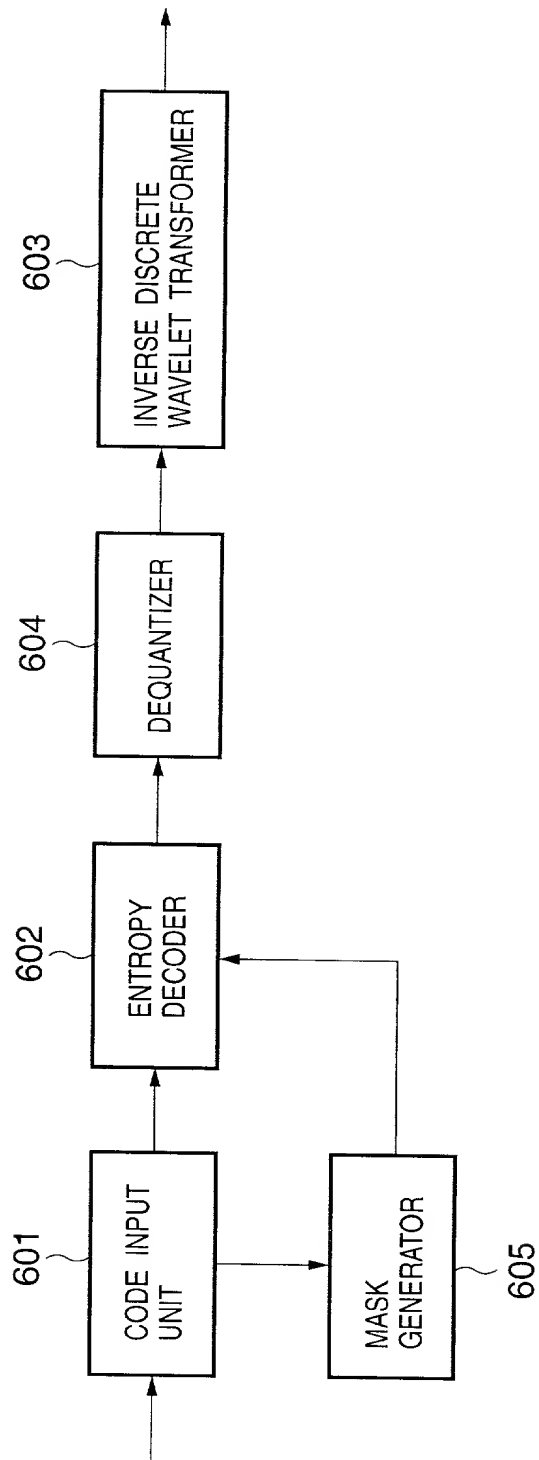


FIG. 23

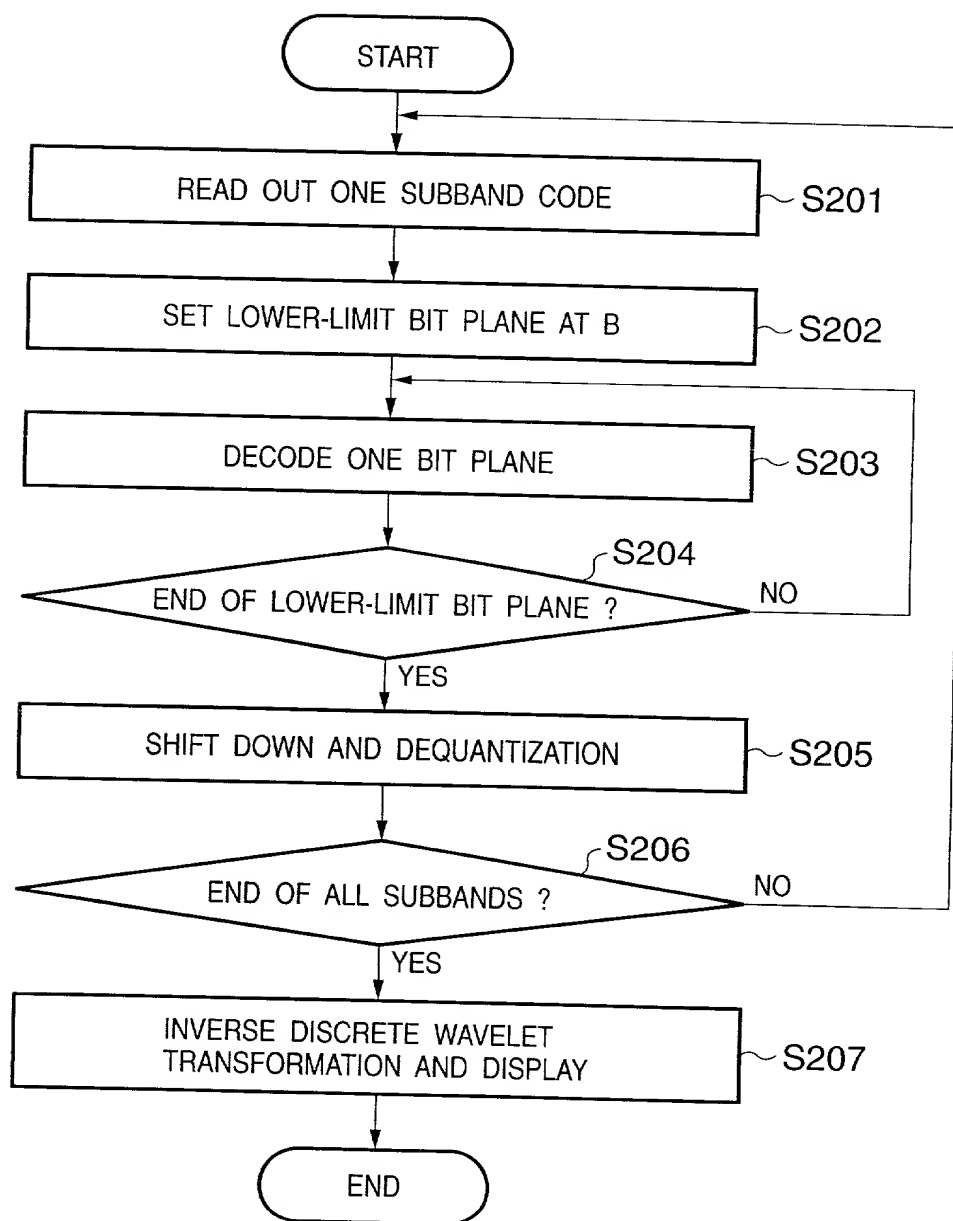


FIG. 24

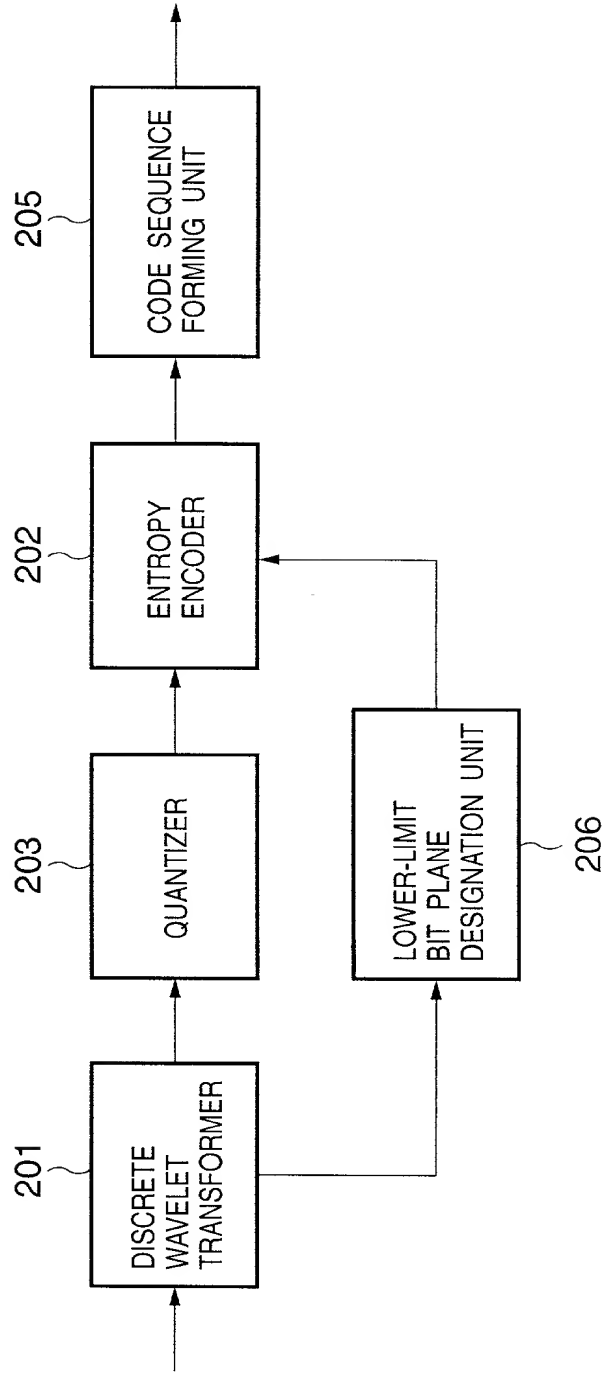


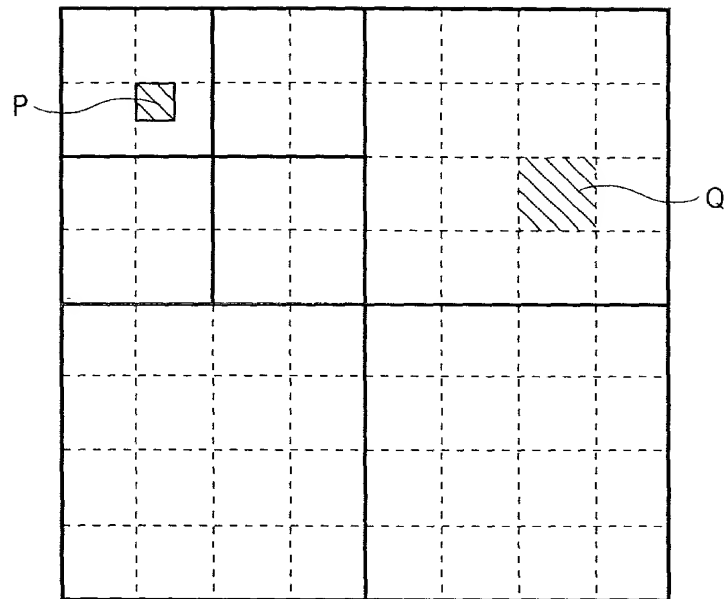
FIG. 25

FIG. 26

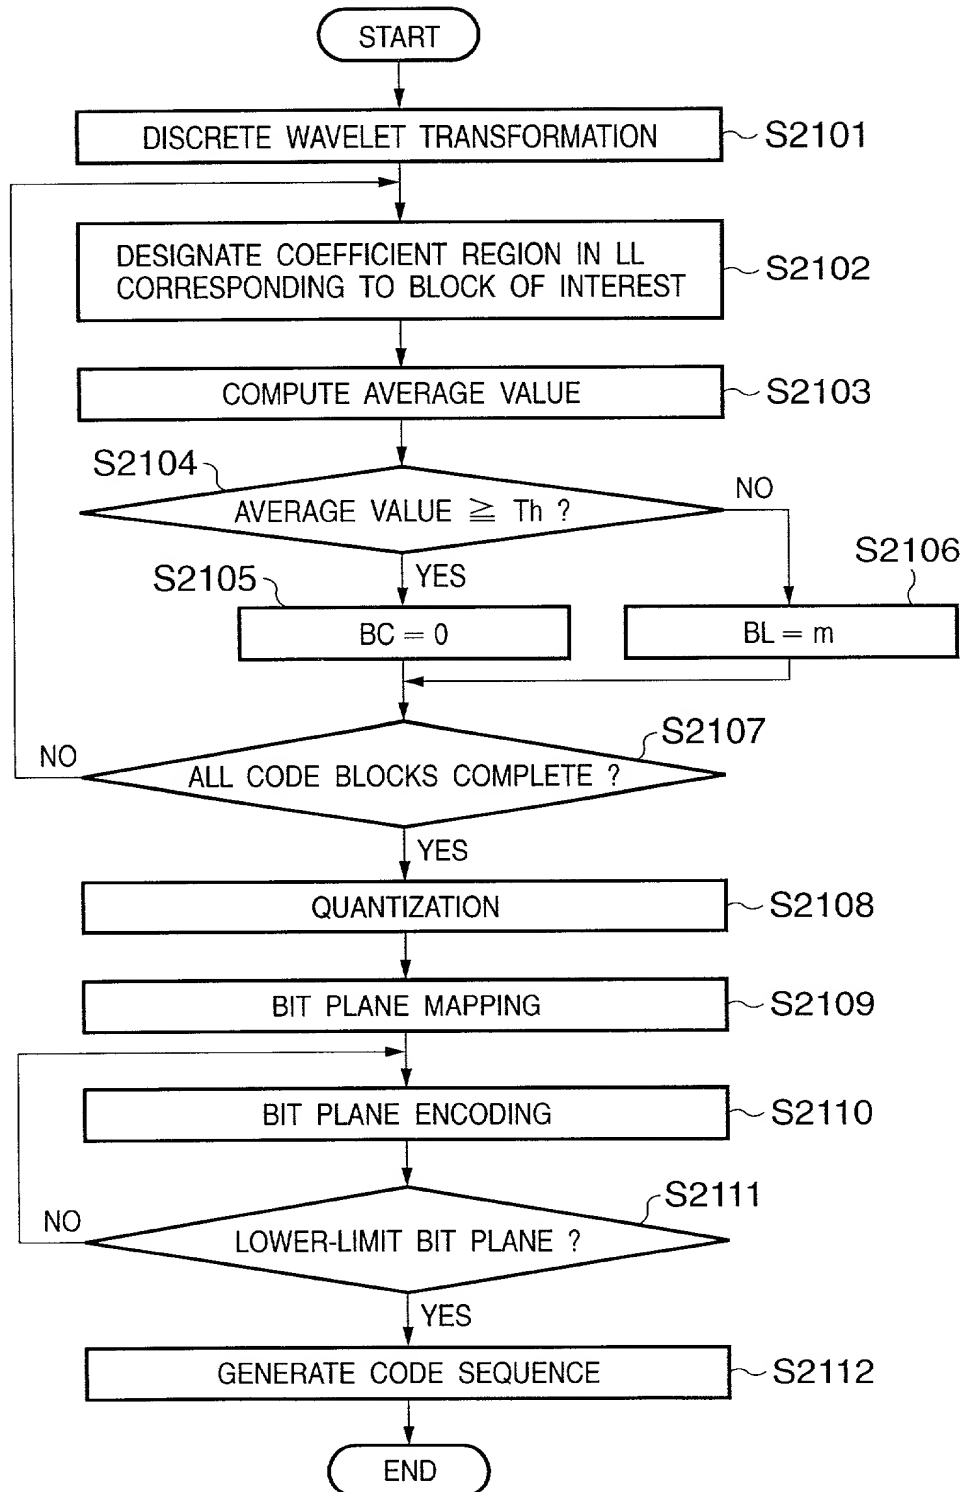


FIG. 27

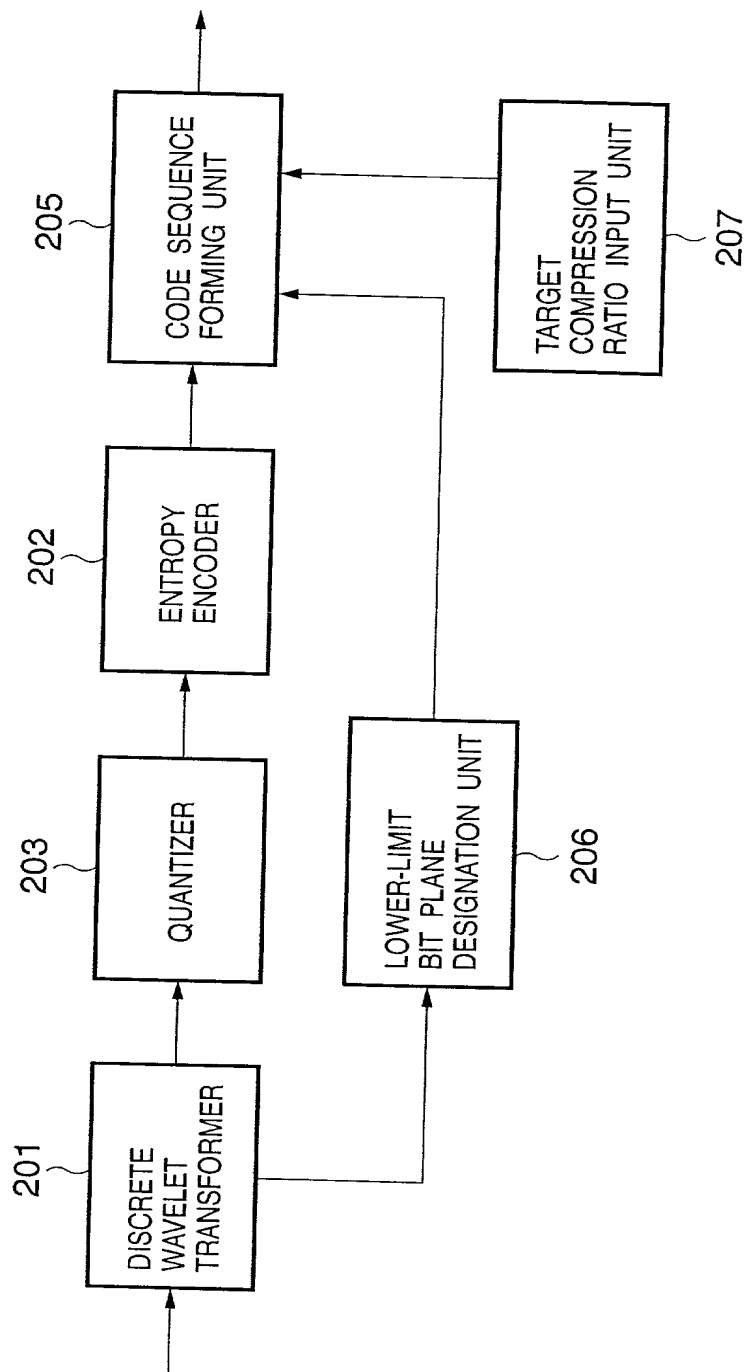


FIG. 28

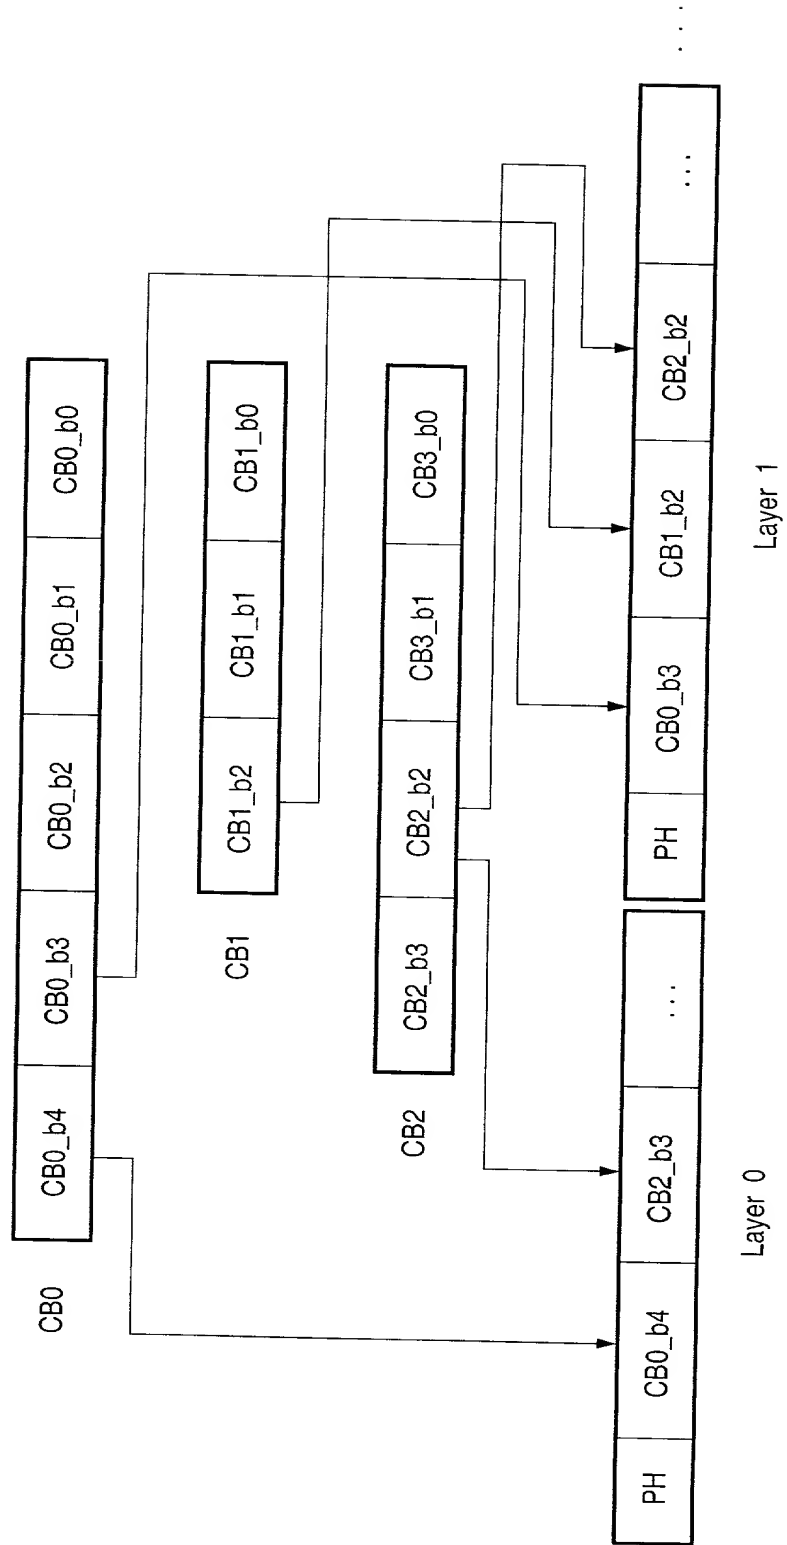


FIG. 29

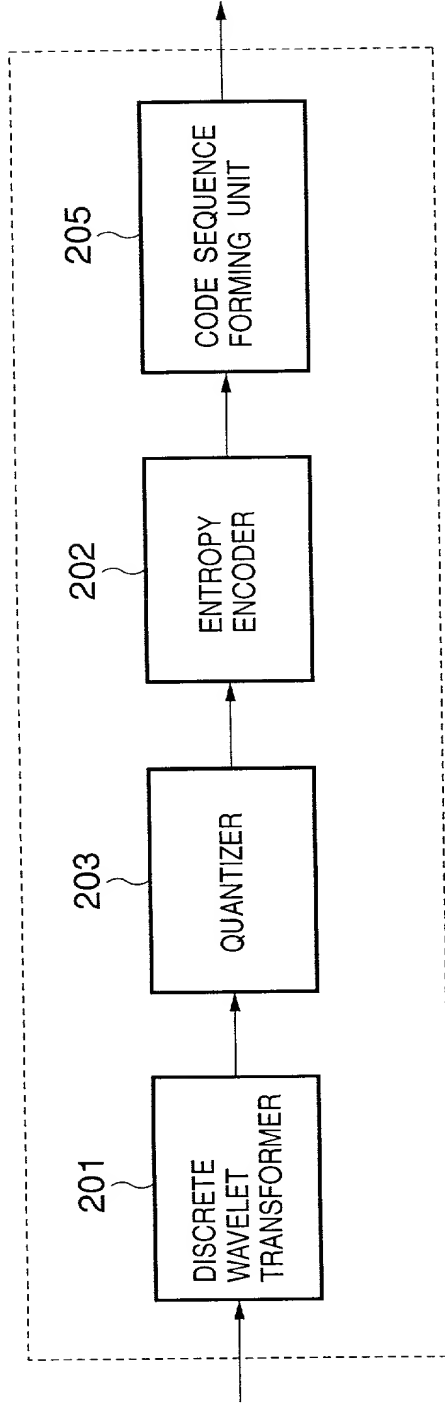


FIG. 30A

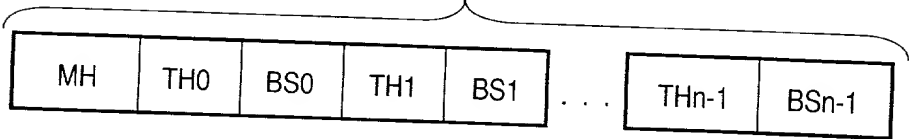


FIG. 30B

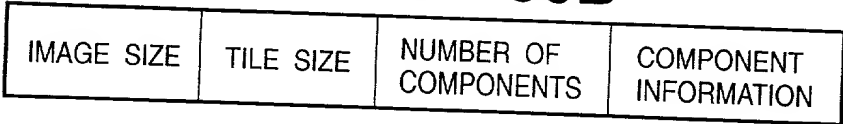


FIG. 30C




FIG. 30D

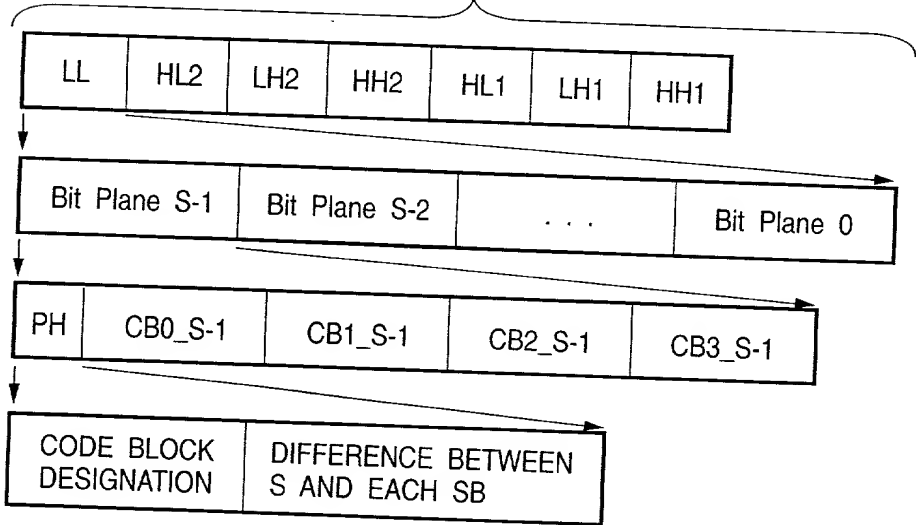


FIG. 30E

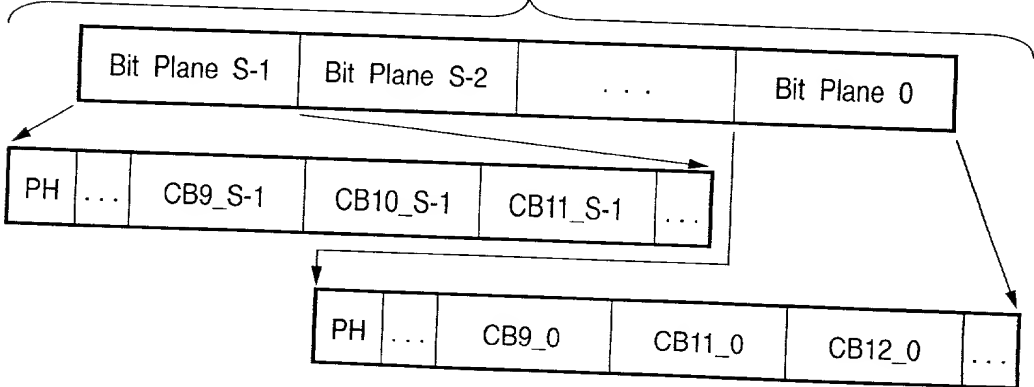


FIG. 31

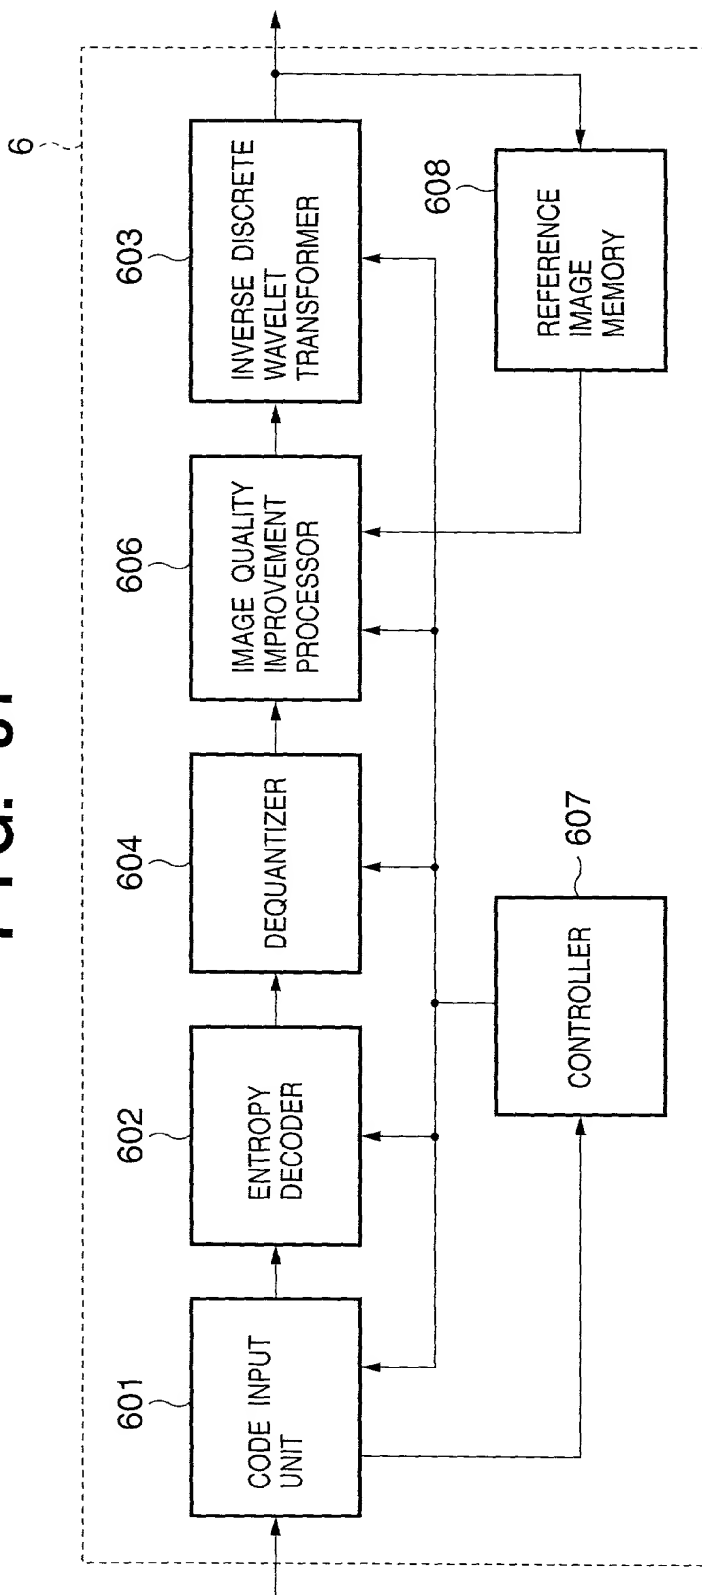


FIG. 32

LL	0	0
0	0	
0		0

FIG. 33

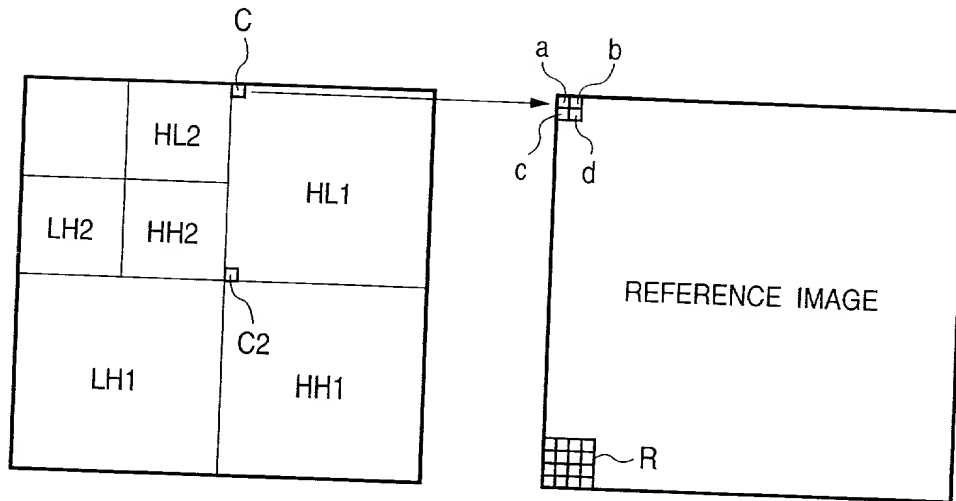


FIG. 34

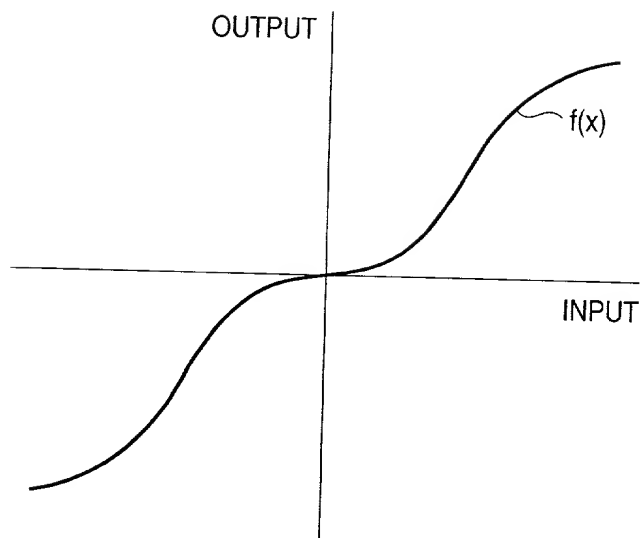


FIG. 35

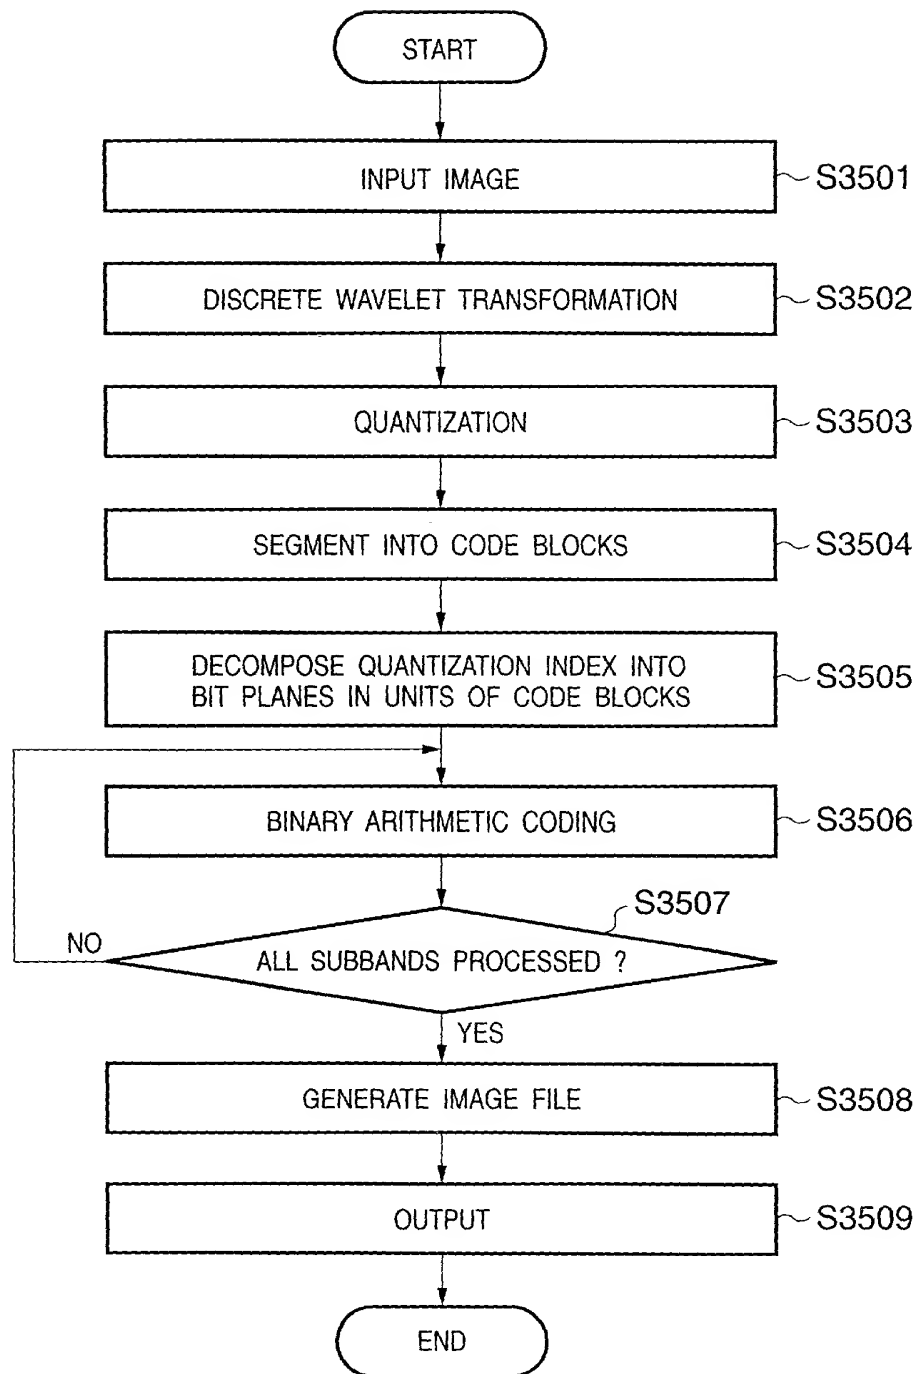


FIG. 35

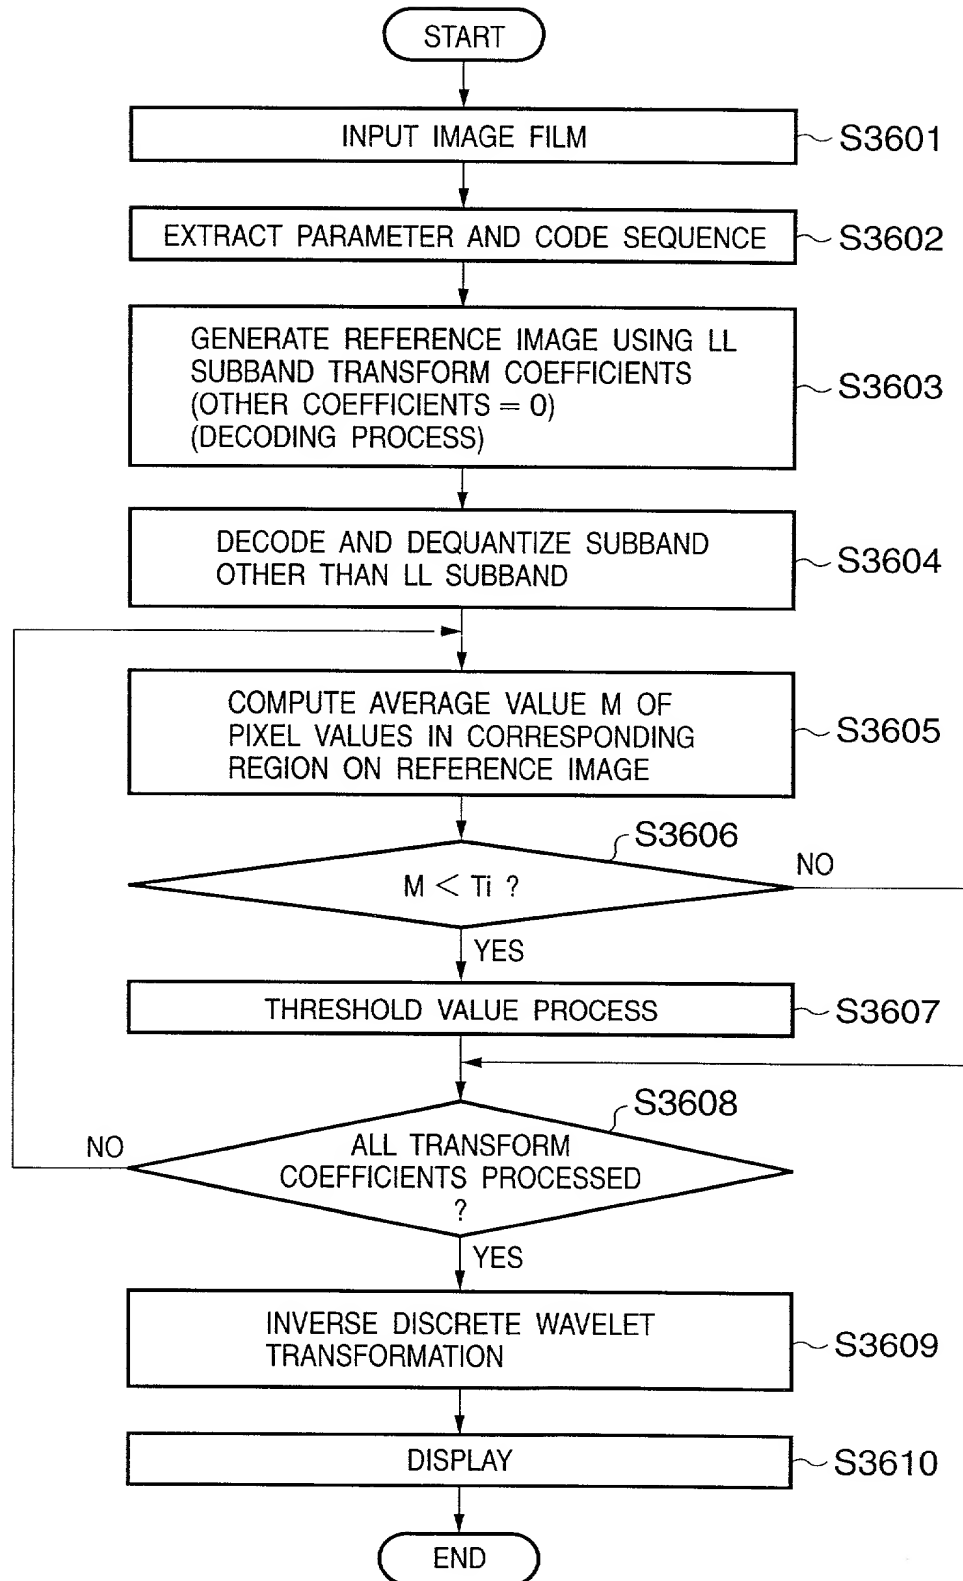
FIG. 36

FIG. 37

LL	HL2	0
LH2	HH2	
0		0

FIG. 37